


## INTENDED USE

The Human Anti-HBsAg IgA ELISA Kit detects and quantifies **HBsAg** (hepatitis B surface antigen) IgA in human serum or plasma or other qualified sample from vaccinated or immunized hosts. This immunoassay is suitable for:

- Determining immune status relative to non-immune controls;
- Assessing efficacy of vaccines, including dosage, adjuvantcy, route of immunization and timing;
- Qualifying and/or standardizing vaccine batches and protocols.

For research use only (RUO), not for diagnosis, cure or prevention of the disease.

## GENERAL INFORMATION




Hepatitis B is an infectious disease caused by hepatitis B virus (HBV). Hepatitis, the acute illness, inflames the liver, causing jaundice, vomiting and (rarely) death. Chronic hepatitis B, however, can cause cirrhosis and liver cancer – a fatal disease. Although viral replication occurs in the liver, HBV spreads to the blood where virus-specific antigens and antibodies may be found in the infected host. Blood tests for these antigens and antibodies are used to diagnose the infection. Acute and chronic hepatitis B can be prevented by vaccination.

HBsAg is the basis for several recent vaccines, which use synthetic recombinant HBsAg and contain no blood products. These vaccines have provided protection for 85-90% of individuals. These vaccines are given intramuscularly. Despite great success, limitations to these vaccines include requirement for refrigeration, multiple injections, thereby reducing wider use. A new nasal hepatitis B vaccine composed of recombinant hepatitis B surface antigen (HBsAg) in a novel nanoemulsion (NE) adjuvant (HBsAg-NE) could be effective with fewer administrations.

Mucosal immunization is an attractive alternative to parenteral vaccines because it can produce both systemic and mucosal immunity and avoids the need for sterile needles. Several mucosal adjuvants (cholera toxin, CpG ODNs, PLG microsphere, and Nano emulsion) have been shown to increase efficacy of nasal vaccines. Immunoglobulin A (IgA, also referred to as sIgA) is an antibody that plays a crucial role in the immune function of mucous membranes. The amount of IgA produced in association with mucosal membranes is greater than all other types of antibody combined. This represents up to ~15% of total Ig's produced throughout the body. sIgA is the main immunoglobulin found in mucous secretions, including tears, saliva, sweat, colostrum and secretions from the genitourinary tract, gastrointestinal tract, prostate and respiratory epithelium. It is also found in small amounts in blood. The secretory component of sIgA protects the immunoglobulin from being degraded by proteolytic enzymes, thus sIgA can survive in the harsh gastrointestinal tract environment and provide protection against microbes that multiply in body secretions. IgA exists in two isotypes, IgA1 and IgA2. Both IgA1 and IgA2 have been found in external secretions like colostrum, maternal milk, tears and saliva, where IgA2 is more prominent than in the blood. Polysaccharide antigens tend to induce more IgA2 than protein antigens.

## PRINCIPLE OF THE TEST



The Human Anti-HBsAg IgA ELISA kit is based on the binding of antibody in samples to HBsAg immobilized on the microwells, and bound antibody is detected by anti-Ig's-specific antibody conjugated to HRP. After a washing step, TMB is added and color (blue) is developed which is directly proportional to the amount of antibody present in the sample. Stopping Solution is added to terminate the reaction, and A450nm is then measured using an ELISA reader. The activity of antibody in samples is determined relative to Calibrators.

## KIT CONTENTS

The microtiter well plate and all other reagents, if unopened, are stable at 2-8°C until the expiration date printed on the box label. Stabilities of the working solutions are indicated under Reagent Preparation.

**To Be Reconstituted:** Store as indicated.

Component	Preparation Instructions
<b>Wash Solution Concentrate (100x)</b> Cat. No. WB-100, 10ml	Dilute the entire volume 10ml + 990ml with distilled or deionized water into a clean stock bottle. Label as <b>Wash Solution</b> and store at ambient temperature until kit is used entirely.
<b>Sample Diluent Concentrate (20x)</b> Cat. No. SD-20T, 10ml	Dilute the entire volume, 10ml + 190ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Sample/Conjugate Diluent (WSD)</b> and store at 2-8°C until the kit lot expires or is used up.
<b>Anti-Human IgA - HRP Conjugate Concentrate (100x)</b> Part No. H-HuA.211, 0.15ml	Supplied in buffer with protein, detergents and antimicrobial as stabilizers. Dilute fresh as needed; 10ul of concentrate to 1ml of <b>Working Sample/Conjugate Diluent</b> is sufficient for 1 8-well strip. Use within the working day and discard. Return 100X to 2-8°C storage.

**Ready For Use:** Store as indicated on labels.

Component	Part	Amt	Contents
<b>HBsAg Microwell Strip Plate</b>	4211	8-well strips (12)	Coated with recombinant HBsAg, and post-coated with stabilizers.
<b>Anti-HBsAg Calibrators</b>			
10 U/ml	4242B	0.65 ml	Four (4) vials, each containing anti-HBsAg in arbitrary activity Units; diluted in buffer with protein, detergents and antimicrobial as stabilizers.
25 U/ml	4242C	0.65 ml	
50 U/ml	4242D	0.65 ml	
100 U/ml	4242E	0.65 ml	
<b>Anti-HbsAg Positive Control</b>	4200-30-PC	0.65ml	Anti-HbsAg IgA; diluted in buffer with protein, detergents and antimicrobial as stabilizers. Net OD > 0.5
<b>Low NSB Sample Diluent</b>	TBTm Not for conjugate dilution	30 ml	Buffer with protein, detergents and antimicrobial as stabilizers. Use as is for sample dilution
<b>TMB Substrate</b>	80091	12 ml	Chromogenic substrate for HRP containing TMB and peroxide.
<b>Stop Solution</b>	80101	12 ml	Dilute sulfuric acid.

### Materials Required But Not Provided:

- Pipettors and pipettes that deliver 100ul and 1-10ml. A multi-channel pipettor is recommended.
- Stock bottle to store diluted Wash Solution; 200ml to 1L.
- Distilled or deionized water to dilute reagent concentrates.
- Microwell plate reader at 450 nm wavelength.

## PRECAUTIONS AND SAFETY INSTRUCTIONS

Calibrators, Sample Diluent, and Antibody HRP contain bromonitrodioxane (BND: 0.05%, w/v). Stop Solution contains dilute sulfuric acid. Follow good laboratory practices, and avoid ingestion or contact of any reagent with skin, eyes or mucous membranes. All reagents may be disposed of down a drain with copious amounts of water. MSDS for TMB, sulfuric acid and BND can be requested or obtained from the ADI website: Sample Diluent and anti-Protein G-HRP contain Proclin 300 (0.05%, v/v). <http://4adi.com/objects/catalog/product/extras/ELISA-Kit-SDS-MSDS-Set-1.pdf>

## LIMITATIONS OF THE ASSAY

### Quantitation of Antibody in a Sample

The ELISA measures anti-HBsAg activity, a combination of antibody concentration and avidity for the HBsAg antigens. Antibodies with substantially different total Ig concentrations may display similar anti-HBsAg activities, due to differences in avidity. The quantitation or activity of the samples is, therefore, appropriately expressed in activity Units (titer), rather than mass units of IgA (e.g., ug/ml).

### Calibrator Curve Quantitation

To quantitate antibody activity from a calibrator curve (such as provided with the kit), the dilution curve of the samples must be parallel to the calibrator curve, to avoid different values being obtained from different regions of the curve. Antibodies that are not matched in HBsAg avidity will often have non-parallel dilution curves. In these cases, antibody activity is best expressed as a titer relative to a reference positive such as the 25 U/ml Calibrator, or another Calibrator in the kit (see Calculation of Results).

## ASSAY DESIGN AND SET-UP

### Sample Collection and Handling

For **serum**, collect blood by venipuncture, allow clotting, and separate the serum by centrifugation at room temperature. For other samples, including **tissue culture media**, clarify the sample by centrifugation and/or filtration prior to dilution in Sample Diluent.

### Sample Dilution & Antibody Stability

Initial dilution of serum into **Working Sample Diluent (WSD)** is recommended to stabilize antibody activity. This enhances reproducible sampling, and stabilizes the antibody activity for years, stored refrigerated or frozen. Further dilution into **Low NSB Sample Diluent (LNSD)**, which provides the lowest assay background, should be at least 10 times the initial dilution and performed the same day as the assay.  
Example: Initial (1/5): 10ul serum + 40ul WSD [or 0.1ml + 0.4ml]  
Further (1/50): 10ul initial (1/5) + 90ul LNSD (1/50)

### Assay Design

Review Calculation of Results (p5-7) and Limits of the Assay (above) before proceeding:

- Select the proper sample dilutions accounting for expected potency of positives and minimizing non-specific binding (NSB) and other matrix effects; for example, net signal for non-immune samples should be <0.5 OD. This is usually 1/50 or greater dilution for human sera with normal levels of IgA and IgM.
- Run a Sample Diluent **Blank**. This signal is an indicator of proper assay performance, especially of washing efficacy, and is used for net OD calculations, if required (**See Method A**).
- Run the Anti-HbsAg Positive Control; net OD > 0.5.
- Run a set of Calibrators. Calibrators validate that the assay was performed to specifications; results can be used to normalize between-assay variation for enhanced precision. Reading values off a Calibrator curve, **Method B**, has limitations. See Limits of the Assay (above).
- Run a range of sample dilutions for expected higher positives that allows calculation of antibody **Titer** (when specific titer is at least 4-fold higher than non-immune). **See Method C**.
- Run samples in duplicate if used for quantitation; non-immunes that are significantly lower than immunes may be run in singlicate. The Calibrators that are used for quantitation, e.g., for between-assay normalization, should be run in duplicate. When determining titer from a dilution curve, singlicates can be run if more than two dilution points are used for titer calculations.

## Plate Set-up

Bring all reagents to room temperature (18-30° C) equilibration (at least 30 minutes).

- Determine the number of wells for the assay run. Duplicates are recommended, including 8 Calibrator wells and 2 wells for each sample and control to be assayed.
- Remove the appropriate number of microwell strips from the pouch and return unused strips to the pouch. Reseal the pouch and store refrigerated.
- Add 200-300ul Working Wash Solution to each well and let stand for about 5 minutes. Aspirate or dump the liquid and pat dry on a paper towel before sample addition.

## Assay Procedure

ALL STEPS ARE PERFORMED AT ROOM TEMPERATURE. After each reagent addition, gently tap the plate to mix the well contents prior to beginning incubation.

- 1st Incubation [100ul – 60 min; 4 washes]**
  - Add 100ul of sample diluent (blank), calibrators, samples and controls each to pre-determined wells.
  - Tap the plate gently to mix reagents and incubate for 60 minutes.
  - Wash wells 4 times and pat dry on fresh paper towels. As an alternative, an automatic plate washer may be used. Improper washes may lead to falsely elevated signals and poor reproducibility.
- 2nd Incubation [100ul – 30 min; 5 washes]**
  - Add 100ul of diluted Antibody-HRP to each well.
  - Incubate for 30 minutes.
  - Wash wells 5 times as in step 2.
- Substrate Incubation [100ul – 15 min]**
  - Add 100ul TMB Substrate to each well. The liquid in the wells will begin to turn blue.
  - Incubate for 15 minutes in the dark, e.g., place in a drawer or closet.

Note: If your microplate reader does not register optical density (OD) above 2.0, incubate for less time, or read OD at 405-410 nm (results are valid).
- Stop Step [Stop: 100ul]**
  - Add 100ul of Stop Solution to each well.
  - Tap gently to mix. The enzyme reaction will stop; liquid in the wells will turn yellow.
- Absorbance Reading**
  - Use any commercially available microplate reader capable of reading at 450nm wavelength. Use a program suitable for obtaining OD readings, and data calculations if available.
  - Read absorbance of the entire plate at 450nm using a single wavelength within 30 minutes after Stop Solution addition. If available, program to subtract OD at 630nm to normalize well background.

## INTERPRETATION OF RESULTS

### Calculation of Results

Consider several data reduction methods to best represent the relationships among experimental and control groups, to determine **Positive Immune** and **Negative Non-immune**, and to **Quantitate** positive antibody levels.

#### Method A. Antibody Activity [ELISA Signal & Sample Dilution]

Represent data as net OD units (A450 signal; blank subtracted) ÷ dilution = **Total Activity Units**.

A Calibrator value in the mid-OD range (e.g., 25 U/ml) can be used to normalize inter-assay values.

#### Method B. Positive Index

Experimental sample values may be expressed relative to the values of Control or Non-immune samples, by calculation of a **Positive Index**. One typical method is as follows:

1. Calculate the net OD mean + 2 SD of the Control/Non-immune samples = **Positive Index**.
2. Divide each sample net OD by the Positive Index. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.

A sample value would be **Positive** if significantly above the value of the pre-immune serum sample or a suitably determined non-immune panel or pool of samples, tested at the same sample dilution. This calculation **quantifies** the positive Antibody Activity level.

#### Example:

Sample	Assay Net OD		Calculated Antibody Activity	
	Control	Exptl	Control	Exptl
1	0.243	2.358	0.49	<b>4.79</b>
2	0.351	0.597	0.71	<b>1.21</b>
3	0.286	1.420	0.58	<b>2.89</b>
4	0.357	1.268	0.73	<b>2.58</b>
5	0.512	0.857	<b>1.04</b>	<b>1.74</b>
6	0.342	1.296	0.70	<b>2.63</b>
7	0.298	0.608	0.61	<b>1.24</b>
8	0.285	0.369	0.58	0.75
9	0.157	0.864	0.32	<b>1.76</b>
10	0.187	0.543	0.38	<b>1.10</b>
Mean	0.302			
SD	0.095			
Mean +2 SD	<b>0.492</b>			<b>= Positive Index</b>

## CALCULATION OF RESULTS (continued)

### Method C. Use of a Calibrator Curve


When the dilution curves of samples are parallel to the Calibrator curve (see Limits of the Assay), the anti-HBsAg activity units may be determined by interpolation from the Calibrator curve, as follows:

1. The results may be calculated using any immunoassay software package. If software is not available, anti-HBsAg activity concentrations may be determined as follows:
2. Calculate the mean OD of duplicate samples.
3. On graph paper plot the mean OD of the calibrators (y-axis) against the concentration (U/ml) of anti-HBsAg (x-axis). Draw the best fit curve through these points to construct the calibrator curve. A point-to-point construction is most common and reliable.
4. The anti-HBsAg activity concentrations in unknown samples and controls can be determined by interpolation from the calibrator curve.
5. Multiply the values obtained for the samples by the dilution factor of each sample.
6. Samples producing signals higher than the 100 U/ml calibrator should be further diluted and re-assayed.

#### Typical Results:

Wells	Calibrators	A450 nm
A1,2	Negative Diluent Blank	0.05
B1,2	10 U/ml Calibrator	0.43
C1,2	25 U/ml Calibrator	0.96
D1,2	50 U/ml Calibrator	1.62
E1,2	100 U/ml Calibrator	2.62
F1,2	Positive Control	1.33

Positive Control Result: = 37 U/ml

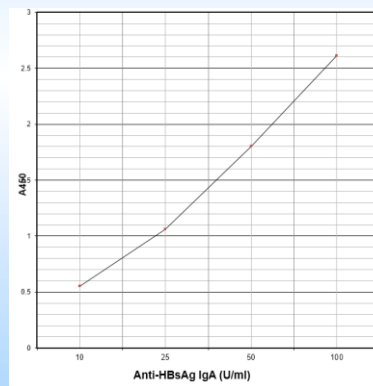

## CALCULATION OF RESULTS (continued)

### Method D. Titers from Sample Dilution Curves

The titer of antibody activity calculated from a dilution curve of each sample is recommended as the most accurate quantitative method. Best precision can be obtained using the following guidelines:


1. Use an OD value Index in the mid-range of the assay (2.0 – 0.5 OD); this provides the best sensitivity and reproducibility for comparing experimental groups and replicates. An arbitrary 1.0 OD is commonly used.
2. Prepare serial dilutions of each sample to provide a series that will produce signals higher and lower than the selected index. With accurate diluting, duplicates may not be required if at least 4 dilutions are run per sample.
3. A 5-fold dilution scheme is useful to efficiently cover a wide range which produces ODs both above and below 1.0 OD. The dilution scheme can be tightened to 3-fold or 2-fold for more precise comparative data.
4. A Calibrator value in the mid-OD range (e.g., 25 U/ml) can be used to normalize inter-assay values.

#### Calculations

1. On a log scale of inverse of Sample Dilution as the x-axis, plot the OD values of the two dilutions of each positive sample having ODs above and below the OD value of the Index (arbitrary or selected Calibrator).
2. From a point-to-point line drawn between the two sample ODs, read the dilution value (x-axis) corresponding to the OD of the selected Index  
= **Total IgA Antibody Activity Units**

#### Example:

II. A 1.0 OD Index was used to determine titer of 4 antibodies.



#### Titer Values

mc154 = 1.72 kU      mc155 = 5.70 kU  
mc156 = 1.85 kU      mc157 = 7.90 kU

#### Assay Sensitivity

The HBsAg -coated plated, the anti-human IgA HRP concentration, and the Low NSB Sample Diluent are optimized to differentiate anti-HBsAg IgA from background (non-antibody) signal with human serum samples diluted 1:50.

#### Calibrator Values

The Calibrators are composed of antibody to HBsAg. Values are assigned as arbitrary anti-HBsAg activity units (see Limits of the Assay).

## PRODUCT SPECIFICATIONS

#### Specificity

Purified recombinant (yeast) HBsAg is used to coat the microwells; thus, no other antibody specificity is detectable in the assay. The anti-human IgA-HRP conjugate specifically detects IgA, and will not react with IgG, IgM or IgE class antibodies. The conjugates detects both IgA1 and IgA2.

# Human Anti-HBsAg IgA ELISA Kit

Cat. No. 4200-30-IGA, 96 tests

For Quantitation of Anti-Hepatitis Surface Antigen (HbsAg) IgA In Serum, Plasma or other Biological samples



For research use only, not for diagnostic or therapeutic use.



**ALPHA DIAGNOSTIC INTERNATIONAL**

6203 Woodlake Center Drive • San Antonio • Texas 78244 • USA.  
Phone (210) 561-9515 • Fax (210) 561-9544  
Toll Free (800) 786-5777

service@4adi.com  
www.4adi.com

Draft version-Please consult the manual supplied with the kit for any lot specific change.