

INTENDED USE

The Mouse anti-dsDNA IgM ELISA Kit is an immunoassay suitable for quantifying or titrating IgM antibody activity specific for dsDNA in serum or plasma. Other biological fluids, including tissue culture medium, may be validated for use. For in vitro research use only (RUO), not for therapeutic or diagnostic use.

GENERAL INFORMATION

Antibodies reactive with autologous nuclear components, such as DNA and histones, can represent an autoimmune basis for pathological conditions such as systemic lupus erythematosus (SLE) in humans, and in mice homozygous for the lymphoproliferation spontaneous mutation (Fas^{lpr}), a systemic autoimmunity with massive lymphadenopathy associated with proliferation of aberrant T cells, arthritis and immune complex glomerulonephritis. These conditions include elevated levels of anti-dsDNA and other anti-nuclear antibodies (ANA) which often increase as the animal ages. Also, the expanded use in the drug industry of biological modifiers has been associated with production of autoantibodies, of which mice, and possibly also other hosts such as humans and monkeys, are susceptible. A prototype disease in mice is lupus caused by the drug minocycline, with elevated anti-dsDNA among other autoantibodies and pathological conditions.

Recent investigations have focused on the role of innate immune mechanisms, including Toll-like receptors (TLRs) and TH2 immunity, responding to the damage-associated molecular patterns of dying cells, as underlying cause of the anti-dsDNA type autoimmunity; these may be induced by drugs, including vaccines and adjuvants, with aging, or with other conditions.

PRINCIPLE OF THE TEST

The Mouse anti-dsDNA IgM ELISA kit is based on the binding of mouse anti-dsDNA IgM in samples to dsDNA immobilized on the microwells, and anti-dsDNA IgM antibody is detected by anti-mouse IgM-specific antibody conjugated to HRP (horseradish peroxidase) enzyme. After a washing step, chromogenic substrate (TMB) is added and color is developed by the enzymatic reaction of HRP on the substrate, which is directly proportional to the amount of anti-dsDNA IgM present in the sample. Stopping Solution is added to terminate the reaction, and absorbance at 450nm is then measured using an ELISA microwell reader. The activity of mouse IgM antibody in samples is calculated relative to anti-DNA calibrators.

PRODUCT SPECIFICATIONS

Specificity

Purified dsDNA is used to coat the microwells; thus the assay is specific for antibodies directed to dsDNA. The anti-Mouse IgM HRP conjugate reacts specifically with mouse IgM class antibodies that bind to dsDNA on the plate. IgA, IgG and IgE antibody would not be measured above background signals.

Assay Sensitivity

The dsDNA coating level, HRP conjugate concentration and Low NSB Sample Diluent are optimized to differentiate anti-dsDNA IgM from background (non-antibody) signal with mouse serum samples diluted 1:100.

Calibrator Values

The calibrators are dilutions of antibody reactive to dsDNA. Values are assigned as arbitrary anti-DNA activity units (see Limits of the Assay).

KIT CONTENTS

The microtiter well plate and all other reagents, if unopened, are stable at 2-8°C until the expiration date printed on the box label. Stabilities of the working solutions are indicated under Reagent Preparation.

To Be Reconstituted: Store as indicated.

| Component | Preparation Instructions |
|--|---|
| Wash Solution Concentrate (100x) Cat. No. WB-100, 10ml | Dilute the entire volume 10ml + 990ml with distilled or deionized water into a clean stock bottle. Label as Working Wash Solution and store at ambient temperature until kit is used entirely. |
| Sample Diluent Concentrate (20x) Cat. No. SD-20T, 10ml | Dilute the entire volume, 10ml + 190ml with distilled or deionized water into a clean stock bottle. Label as Working Sample Diluent and store at 2-8°C until the kit lot expires or is used up. |
| Anti-Mouse IgM- HRP Conjugate Concentrate (100x) Part: H-MsM.612, 0.15ml | Peroxidase conjugated anti-Mouse IgM in buffer with protein, detergents and antimicrobial as stabilizers. Dilute fresh as needed; 10ul of concentrate to 1ml of Working Sample Diluent (WSD) is sufficient for 1 8-well strip. Use within the working day and discard. Return 100X to 2-8°C storage. |

Ready For Use: Store as indicated on labels.


| Component | Part | Amt | Contents |
|--|---------|--------------------|---|
| dsDNA Microwell Strip Plate | 5101 | 8-well strips (12) | Coated with dsDNA, and post-coated with stabilizers. |
| Anti-DNA Calibrators | | | |
| 50 U/ml | 51d53sB | 0.65 ml | Four (4) vials, each containing anti-DNA IgM levels in arbitrary activity Units; diluted in buffer with protein, detergents and antimicrobial as stabilizers. |
| 200 U/ml | 51d53sC | 0.65 ml | |
| 500 U/ml | 51d53sD | 0.65 ml | |
| 1000 U/ml | 51d53sE | 0.65 ml | |
| Low NSB Sample Diluent (LNSD) Reduces non-specific binding | TBTm | 30 ml | Buffer with protein, detergents and antimicrobial as stabilizers. Use as is for sample dilution. See Assay Design , page 3. Not for HRP Conjugate dilution. |
| TMB Substrate | 80091 | 12 ml | Chromogenic substrate for HRP containing TMB and peroxidase. |
| Stop Solution | 80101 | 12 ml | Dilute sulfuric acid. |

Materials Required But Not Provided:

- Pipettors and pipettes that deliver 100ul and 1-10ml. A multi-channel pipettor is recommended.
- Disposable glass or plastic 5-15ml tubes for diluting samples and Anti-Mouse IgM HRP Concentrate.
- Graduated cylinder to dilute Wash Concentrate; 0.2 to 1L.
- Stock bottle to store diluted Wash Solution; 0.2 to 1L.
- Distilled or deionized water to dilute reagent concentrates.
- Microwell plate reader at 450 nm wavelength.

ASSAY DESIGN AND SET-UP

The **Low NSB Sample Diluent**, TBTm, lowers NSB even more than does the 1xSD20T Diluent, without diminishing true positive antibody signals, thus offering a greater discrimination between positives and non-immune samples.

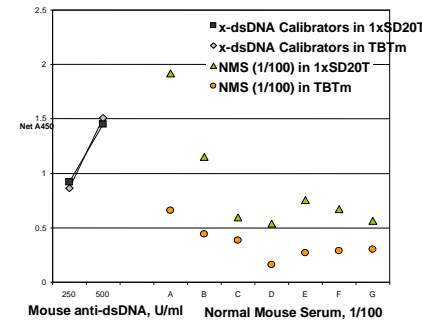

Sample Collection and Handling

Culture medium, serum and other biological fluids may be used as samples with proper dilution to avoid solution matrix interference. For **serum**, collect blood by venipuncture, allow clotting, and separate the serum by centrifugation at room temperature. For other samples, including **tissue culture media**, clarify the sample by centrifugation and/or filtration prior to dilution in Sample Diluent.

Antibody Stability

Initial dilution of serum into **Working Sample Diluent (WSD)** is recommended to stabilize antibody activity. This enhances reproducible sampling, and stabilizes the antibody activity for years, stored refrigerated or frozen. Further dilution into **Low NSB Sample Diluent (LNSD)**, which provides the lowest assay background, should be at least 10 times the initial dilution and performed the same day as the assay.

Example: Initial (1/5): 10ul serum + 40ul WSD [or 0.1ml + 0.4ml]
Further (1/50): 10ul initial (1/5) + 90ul LNSD (1/50)

Assay Design

Review Calculation of Results (p5-7) and Limits of the Assay (above) before proceeding:

- **Select the proper sample dilutions.** Account for expected potency of positives and minimize non-specific binding (NSB) and other matrix effects; for example, non-immune samples should give net signal <0.5 OD. This is usually 1/100 or greater dilution for mouse sera with normal levels of IgG and IgM. Dilute samples in **Working Sample Diluent (1xSD20T)** or in **Low NSB Sample Diluent (TBTm)** (see above). Note: **all samples** must be diluted in the same diluent for proper comparison – either TBTm or 1xSD20T.
- Run a Sample Diluent **Blank**. This signal is an indicator of proper assay performance, especially of washing efficacy, and is used for net OD calculations, if required. Blank OD should be <0.3. **See Method A and B.**
- Run a set of Calibrators. Calibrators validate that the assay was performed to specifications, and can be used to normalize between-assay variation for enhanced precision. Reading values off a Calibrator curve, **Method C**, has limitations. See Limits of the Assay above.
- Run a range of sample dilutions for expected higher positives that allows calculation of antibody **Titer** (when specific titer is at least 4-fold higher than non-immune). **See Method D.**
- Run samples in duplicate if used for quantitation; non-immunes that are significantly lower than immunes may be run in singlicate. The Calibrators that are used for quantitation, e.g., for between-assay normalization, should be run in duplicate. When determining titer from a dilution curve, singlicates can be run if more than two dilution points are used for titer calculations.

Bring all reagents to room temperature (18-30° C) equilibration (at least 30 minutes).

- Determine the number of wells for the assay run. Duplicates are recommended, including 8 Calibrator wells and 2 wells for each sample and control to be assayed.
- Remove the appropriate number of microwell strips from the pouch and return unused strips to the pouch. Reseal the pouch and store refrigerated.
- Add 200-300ul Working Wash Solution to each well and let stand for about 5 minutes. Aspirate or dump the liquid and pat dry on a paper towel before sample addition.

Assay Procedure

ALL STEPS ARE PERFORMED AT ROOM TEMPERATURE. After each reagent addition, gently tap the plate to mix the well contents prior to beginning incubation.

1. 1st Incubation [100ul – 60 min; 4 washes]

- Add 100ul of sample diluent (blank) calibrators, samples and controls each to pre-determined wells.
- Tap the plate gently to mix reagents and incubate for 60 minutes.
- Wash wells 4 times and pat dry on fresh paper towels. As an alternative, an automatic plate washer may be used. Improper washes may lead to falsely elevated signals and poor reproducibility.

2. 2nd Incubation [100ul – 30 min; 5 washes]

- Add 100ul of diluted Anti-Mouse IgM HRP to each well.
- Incubate for 30 minutes.
- Wash wells 5 times as in step 2.

3. Substrate Incubation [100ul – 15 min]

- Add 100ul TMB Substrate to each well. The liquid in the wells will begin to turn blue.
- Incubate for 15 minutes in the dark, e.g., place in a drawer or closet.

Note: If your microplate reader does not register optical density (OD) above 2.0, incubate for less time, or read OD at 405-410 nm (results are valid).

4. Stop Step [Stop: 100ul]

- Add 100ul of Stop Solution to each well.
- Tap gently to mix. The enzyme reaction will stop; liquid in the wells will turn yellow.

5. Absorbance Reading

- Use any commercially available microplate reader capable of reading at 450nm wavelength. Use a program suitable for obtaining OD readings, and data calculations if available.
- Read absorbance of the entire plate at 450nm using a single wavelength within 30 minutes after Stop Solution addition. If available, program to subtract OD at 630nm to normalize well variation.

The ELISA measures anti-dsDNA activity, a combination of antibody concentration and avidity for the dsDNA antigens. Antibodies with substantially different IgM concentrations may display similar anti-dsDNA activities, due to differences in avidity. The quantitation or activity of the samples is, therefore, appropriately expressed in activity Units (titer), rather than mass units of IgM (e.g., ug/ml).

Calibrator Curve Quantitation

To quantitate antibody activity from a calibrator curve (such as provided with the kit, **Method C**, the dilution curve of the samples must be parallel to the calibrator curve, to avoid different values being obtained from different regions of the curve. Antibodies that are not matched in anti-dsDNA avidity will often have non-parallel dilution curves. In these cases, antibody activity is best expressed as **Method A**: ELISA value & dilution; **Method B**: a multiple of a Positive Index titer; or **Method D**: anti-dsDNA titer from a sample dilution curve (see Calculation of Results).

INTERPRETATION OF RESULTS

Calculation of Results

Consider several data reduction methods to best represent the relationships among experimental and control groups, to determine **Positive Immune** and **Negative Non-immune**, and to **Quantitate** positive antibody levels.

Method A. Antibody Activity [ELISA Signal & Sample Dilution]
Represent data as net OD units (A450 signal; blank subtracted) ÷ dilution = **Total Activity Units**.

A Calibrator value in the mid-OD range (e.g., 200 U/ml) can be used to normalize inter-assay values.

Method B. Positive Index

Experimental sample values may be expressed relative to the values of Control or Non-immune samples, by calculation of a **Positive Index**. One typical method is as follows:

1. Calculate the net OD mean + 2 SD of the Control/Non-immune samples = **Positive Index**.
2. Divide each sample net OD by the Positive Index. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.

A sample value would be **Positive** if significantly above the value of the pre-immune serum sample or a suitably determined non-immune panel or pool of samples, tested at the same sample dilution. This calculation **quantifies** the positive Antibody Activity level.

Example:

| Sample | Assay Net OD | | Calculated Antibody Activity | |
|------------|--------------|-------|------------------------------|-------------------------|
| | Control | Exptl | Control | Exptl |
| 1 | 0.243 | 2.358 | 0.49 | 4.79 |
| 2 | 0.351 | 0.597 | 0.71 | 1.21 |
| 3 | 0.286 | 1.421 | 0.58 | 2.89 |
| 4 | 0.357 | 1.268 | 0.73 | 2.58 |
| 5 | 0.512 | 0.857 | 1.04 | 1.74 |
| 6 | 0.342 | 1.296 | 0.70 | 2.63 |
| 7 | 0.298 | 0.608 | 0.61 | 1.24 |
| 8 | 0.285 | 0.369 | 0.58 | 0.75 |
| 9 | 0.157 | 0.864 | 0.32 | 1.76 |
| 10 | 0.187 | 0.543 | 0.38 | 1.10 |
| Mean | 0.302 | | | |
| SD | 0.095 | | | |
| Mean +2 SD | 0.492 | | | = Positive Index |

PRECAUTIONS AND SAFETY INSTRUCTIONS

Calibrators, Sample Diluent, and Antibody HRP contain bromonitrodioxane (BND: 0.05%, w/v). Stop Solution contains dilute sulfuric acid. Follow good laboratory practices, and avoid ingestion or contact of any reagent with skin, eyes or mucous membranes. All reagents may be disposed of down a drain with copious amounts of water. MSDS for TMB, sulfuric acid and BND can be requested or obtained from the ADI website: http://www.4adi.com/commerce/info/showpage.jsp?page_id=1060&category_id=2430&visit=10

Method C. Use of a Calibrator Curve


When the dilution curves of samples are parallel to the Calibrator curve (see Limits of the Assay), the anti-dsDNA activity units may be determined by interpolation from the Calibrator curve. The results may be calculated using any immunoassay software package. If software is not available, anti-dsDNA activity concentrations may be determined as follows:

1. Calculate the mean OD of duplicate samples.
2. On graph paper plot the mean OD of the calibrators (y-axis) against the concentration (U/ml) of anti-dsDNA (x-axis). Draw the best fit curve through these points to construct the calibrator curve. A point-to-point construction is most common and reliable.
3. The anti-dsDNA activity concentrations in unknown samples and controls can be determined by interpolation from the calibrator curve.
4. Multiply the values obtained for the samples by the dilution factor of each sample.
5. Samples producing signals higher than the 1000 U/ml calibrator should be further diluted and re-assayed.

Typical Results:

| Wells | Calibrators | A450 nm |
|-------|------------------------|---------|
| A1,2 | Negative Diluent Blank | 0.03 |
| B1,2 | 50 U/ml Calibrator | 0.37 |
| C1,2 | 200 U/ml Calibrator | 1.17 |
| D1,2 | 500 U/ml Calibrator | 2.35 |
| E1,2 | 1000 U/ml Calibrator | 2.83 |
| F1,2 | Sample 1:100 | 1.61 |

Sample Result: 280 U/ml x 100 dilution = **28.0 kU/ml**

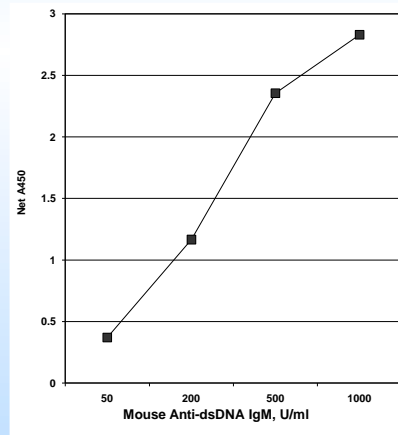

Method D. Titers from Sample Dilution Curves

The titer of antibody activity calculated from a dilution curve of each sample is recommended as the most accurate quantitative

method. Best precision can be obtained using the following guidelines:


1. Use an OD value Index in the mid-range of the assay (2.0 – 0.5 OD); this provides the best sensitivity and reproducibility for comparing experimental groups and replicates. An arbitrary 1.0 OD is commonly used.
2. Prepare serial dilutions of each sample to provide a series that will produce signals higher and lower than the selected index. With accurate diluting, duplicates may not be required if at least 4 dilutions are run per sample.
3. A 5-fold dilution scheme is useful to efficiently cover a wide range which produces ODs both above and below 1.0 OD. The dilution scheme can be tightened to 3-fold or 2-fold for more precise comparative data.
4. A Calibrator value in the mid-OD range (e.g., 200 U/ml) can be used to normalize inter-assay values.

Calculations

1. On a log scale of inverse of Sample Dilution as the x-axis, plot the OD values of the two dilutions of each positive sample having ODs above and below the OD value of the Index (arbitrary or selected Calibrator).
2. From a point-to-point line drawn between the two sample ODs, read the dilution value (x-axis) corresponding to the OD of the selected Index
= Total IgM Antibody Activity Units

Example:

II. A 1.0 OD Index was used to determine titer of 4 antibodies.

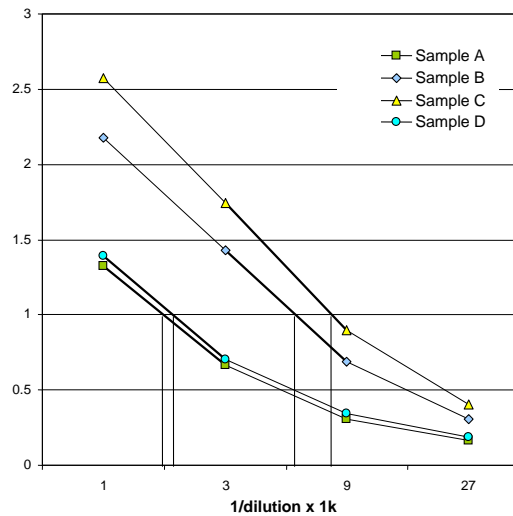

| Titer Values | |
|--------------|-----------|
| Sample A | = 1.72 kU |
| Sample B | = 5.70 kU |
| Sample C | = 1.85 kU |
| Sample D | = 7.90 kU |

Mouse Anti-dsDNA IgM ELISA Kit

Cat. No. 5130

For Quantitation of anti-dsDNA IgM in Serum or plasma



ALPHA DIAGNOSTIC INTERNATIONAL

4638 N Loop 1604 West • San Antonio • Texas 78249 • USA.

Phone (210) 561-9515 • Fax (210) 561-9544

Toll Free (800) 786-5777

Email: service@4adi.com
www.4adi.com

| ELISA Kit Components | Amount | Part |
|-------------------------------------|--------------------|-----------|
| dsDNA Coated Microwell Strip Plate | 8-well strips (12) | 5101 |
| Anti-DNA Calibrator | 50 U/ml 0.65 ml | 51d53sB |
| Anti-DNA Calibrator | 200 U/ml 0.65 ml | 51d53sC |
| Anti-DNA Calibrator | 500 U/ml 0.65 ml | 51d53sD |
| Anti-DNA Calibrator | 1000 U/ml 0.65 ml | 51d53sE |
| Anti-Mouse IgM HRP Conjugate (100X) | 0.15 ml | H-MsM.612 |
| Sample Diluent (20x) | 10 ml | SD20T |
| Low NSB Sample Diluent | 30 ml | TBTm |
| Wash Solution Concentrate (100X) | 10 ml | WB-100 |
| TMB Substrate | 12 ml | 80091 |
| Stop Solution | 12 ml | 80101 |
| Product Manual | 1 ea | M-5130 |