

## INTENDED USE

The Rabbit Anti-Pneumococcal CPS23 IgG ELISA Kit quantifies IgG antibodies against capsular polysaccharides (CPS) of 23 serotypes (Pneumovax vaccine) in serum/plasma of vaccinated or normal hosts. This immunoassay is suitable for:

- Determining **immune status** relative to controls;
  - Assessing efficacy of **vaccines**, including dosage, adjuvantcy, route of immunization and timing;
  - Qualifying and standardizing vaccine batches & protocols.
- This kit is for research use only (RUO).

## GENERAL INFORMATION



*Streptococcus pneumoniae*, or pneumococcus, a Gram-positive bacteria, is one of the most common causes, along with *N. meningitidis*, of bacterial meningitis in adults and young adults. Pneumococcal strains have capsular polysaccharides (CPS)

that act as a virulence factor for the organism; more than 90 different serotypes are known. Serotype specific antibodies against the CPS provide protection against the corresponding strains. The pneumococcal vaccine most commonly used today consists of purified polysaccharides from **23 serotypes** (1, 2, 3, 4, 5, 6B, 7F, 8, 9N, 9V, 10A, 11A, 12F, 14, 15B, 17F, 18C, 19F, 19A, 20, 22F, 23F and 33F; non-conjugated: **Pneumovax** by Merck). Pneumococcal conjugate vaccines (PCV) contain polysaccharides conjugated to diphtheria toxin **CRM197**, with three PCV vaccines currently available: **Prenvar-7** or **PCV-7** (Wyeth) is a 7-valent vaccine (4, 6B, 9V, 14, 18C, 19F, and 23F); **Synflorix** (GlaxoSmithKline) is a 10-valent vaccine (PCV-10: 1, 4, 5, 6B, 7F, 9V, 14, 18C, 19F, and 23F); **Prenvar-13** (Pfizer) is 13-valent (PCV-13: 1, 3, 4, 5, 6A, 6B, 7F, 9V, 14, 18C, 19A, 19F, 23F); each are conjugated to carrier protein CRM197.

## PRINCIPLE OF THE TEST

The Anti-CPS23 IgG ELISA kit is based on the binding of anti-CPS Ig's in samples to the purified CPS antigens coated on the microwells; bound antibodies are detected by specific antibody-HRP conjugate (species and isotype specific). After a washing step, substrate (TMB) is added and color (blue) is developed, which is directly proportional to the amount of antibody present in the samples. Stopping Solution is added to terminate the reaction, A450nm (yellow color) is then measured using an ELISA reader. The activity of anti-CPS IgG in samples is determined relative to anti-CPS specific Calibrators.

## PRODUCT SPECIFICATIONS

### Specificity

The plate is coated with a mixture of 23 purified non-conjugated CPS of pneumovax vaccine; no antibodies to CRM197 will be detected. These CPS preparations are contaminated with **CWPS** (Cell Wall Polysaccharide), which is common to all pneumococci, both virulent and avirulent strains. An **adsorption step** may be required to remove these antibodies prior to testing for antibodies to the CPS (#560-420-C22). The antibody-HRP conjugate specifically detects IgG, and does not react with IgM, IgA or IgE class antibodies. ADI has other ELISA kits to detect antibodies to PCV7, PCV10, PCV23 or other vaccines.

### Assay Sensitivity

The CPS23-coated plate, anti-Human IgG HRP concentration, and Low NSB Sample Diluent are optimized to differentiate anti-CPS23 IgG from control and immune animals when samples are tested at a dilution of 1:100 or higher.

## KIT CONTENTS

The microtiter well plate and all other reagents, if unopened, are stable at 2-8° C until the expiration date printed on the box label. Stabilities of the working solutions are indicated under Reagent Preparation.

**To Be Reconstituted:** Store as indicated.

Component	Preparation Instructions
<b>Wash Solution Concentrate (100x)</b> Cat. No. WB-100, 10ml	Dilute the entire volume 10ml + 990ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Wash Solution</b> and store at 4°C for long term and RT for short term.
<b>Sample Diluent Concentrate (20x)</b> Cat. No. SD-20T, 10ml	Dilute the entire volume, 10ml + 190ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Sample/Conjugate Diluent (WSD)</b> and store at 2-8°C until the kit lot expires or is used up.
<b>Anti-Rabbit IgG-HRP Conjugate Concentrate (100x)</b> Part: H-RuG.211, 0.15ml	In buffer with detergents and antimicrobial. Dilute fresh as needed; 10ul of concentrate to 1ml of <b>Working Sample/Conjugate Diluent</b> is sufficient for 1 8-well strip. Use within the working day and discard. Return 100X to 2-8° C storage.

**Ready For Use:** Store as indicated on labels.

Component	Part	Amt	Contents
<b>CPS 23 Type CPS Coated Strip Plate</b>	560-23	8-well strips (12)	Coated with 23 serotypes of CPS antigen,
<b>Anti-Pneumococcal Calibrators</b>			
1 U/ml	560-07rSB	0.65ml	Four (4) vials, each containing anti-pneumococcal CPS; in buffer with antimicrobial.
2.5 U/ml	560-07rSC	0.65ml	
5 U/ml	560-07rSD	0.65ml	
10 U/ml	560-07rSE	0.65ml	
<b>Rabbit Anti-Pneumococcal 23 IgG Positive Control</b>	560-190-PC	0.65ml	Anti-CPS IgG; diluted in buffer with protein, detergents and antimicrobial. Net OD > 0.5
<b>Low NSB Sample Diluent (LNSB)</b> Reduces non-specific binding	TBTm  Not for HRP Conjugate dilution	30 ml	Buffer with protein, detergents and antimicrobial.  Use as is for sample dilution. See <b>Assay Design</b> , page 3.
<b>TMB Substrate</b>	80091	12 ml	Chromogenic substrate for HRP containing TMB and peroxide.
<b>Stop Solution</b>	80101	12 ml	Dilute sulfuric acid.

### Materials Required But Not Provided:

- Pipettors and pipettes that deliver 100ul and 1-10ml.
- Disposable glass or plastic 5-15ml tubes
- Distilled or deionized water to dilute reagent concentrates.
- ELISA reader at 450 nm and ELISA plate washer

## ASSAY DESIGN AND SET-UP

### Sample Collection and Handling

Serum and other biological fluids may be used as samples with proper dilution to avoid solution matrix interference. For **serum**, collect blood by venipuncture, allow clotting, and separate the serum by centrifugation at room temperature. If samples will not be assayed immediately, store refrigerated for up to a few weeks, or frozen for long-term storage.

### Antibody Stability

Initial dilution of serum into **Working Sample Diluent (WSD)** is recommended to stabilize antibody activity. This enhances reproducible sampling, and stabilizes the antibody activity for years, stored refrigerated or frozen. Further dilution into **Low NSB Sample Diluent (LNSB)**, which provides the lowest assay background, should be at least 5 times the initial dilution and performed the same day as the assay.

### Assay Design

Review Interpretation of Results (p5-7) before proceeding:

- Pre-adsorb samples with **CWPS/22F** antigen, if necessary (see Specificity, page 1)
- Select the proper sample dilutions accounting for expected potency of positives and minimizing non-specific binding (NSB) and other matrix effects; for example, net signal for non-immune samples should be lower than the **1 U/ml Calibrator**. This is usually 1/100 or greater dilution for human serum with normal levels of IgG and IgM.
- Run a Sample Diluent **Blank**. This signal is an indicator of proper assay performance, especially of washing efficacy, and is used for net OD calculations, if required. Blank OD should be <0.3.
- Run the Human Anti-Pneumococcal 23 IgG **Positive Control**; net OD > 0.5.
- Run a set of **Calibrators**, which validate that the assay was performed to specifications: **10 U/ml** should give a high signal (>1.5 OD); **1 U/ml** should give a low signal which can be used to discriminate at the Positive/Negative threshold (see Interpretation of Results, p. 5).

### Plate Set-up

Bring all reagents to room temperature (18-30° C) equilibration (at least 30 minutes).

- Determine the number of wells for the assay run. Duplicates are recommended, including 8 Calibrator wells and 2 wells for each sample control to be assayed.
- Remove the appropriate number of microwell strips from the pouch and return unused strips to the pouch. Reseal the pouch and store refrigerated.
- Add 200-300ul Working Wash Solution to each well and let stand for about 5 minutes. Aspirate or dump the liquid and pat dry on a paper towel before sample addition.

## Assay Procedure

ALL STEPS ARE PERFORMED AT ROOM TEMPERATURE. After each reagent addition, gently tap the plate to mix the well contents prior to beginning incubation.

- 1st Incubation [100ul – 60 min; 4 washes]**
  - Add 100ul of sample diluent (blank), calibrators, samples and controls each to pre-determined wells.
  - Tap the plate gently to mix reagents and incubate for 60 minutes.
  - Wash wells 4 times and pat dry on fresh paper towels. As an alternative, an automatic plate washer may be used. Improper washes may lead to falsely elevated signals and poor reproducibility.
- 2nd Incubation [100ul – 30 min; 5 washes]**
  - Add 100ul of diluted Anti-Human IgG HRP to each well.
  - Incubate for 30 minutes.
  - Wash wells 5 times as in step 2.
- Substrate Incubation [100ul – 15 min]**
  - Add 100ul TMB Substrate to each well. The liquid in the wells will begin to turn blue.
  - Incubate for 15 minutes in the dark, e.g., place in a drawer or closet.

Note: If your microplate reader does not register optical density (OD) above 2.0, incubate for less time, or read OD at 405-410 nm (results are valid).
- Stop Step [Stop: 100ul]**
  - Add 100ul of Stop Solution to each well.
  - Tap gently to mix. The enzyme reaction will stop; liquid in the wells will turn yellow.
- Absorbance Reading**
  - Use any commercially available microplate reader capable of reading at 450nm wavelength. Use a program suitable for obtaining OD readings, and data calculations if available.
  - Read absorbance of the entire plate at 450nm using a single wavelength within 30 minutes after Stop Solution addition. If available, program to subtract OD at 630nm to normalize well background.

# Rabbit Anti-Pneumococcal CPS23 IgG ELISA Kit

Cat#. 560-310-23G, 96 tests

For Quantitation of Anti-CPS IgG to 23 Serotypes (1, 2, 3, 4, 5, 6B, 7F, 8, 9N, 9V, 10A, 11A, 12F, 14, 15B, 17F, 18C, 19F, 19A, 20, 22F, 23F and 33F) in Serum or Plasma

For research use only, not for diagnostic or therapeutic use.



**ALPHA DIAGNOSTIC INTERNATIONAL**

6203 Woodlake Center Drive  
San Antonio, Texas 78244 • USA.  
Phone (210) 561-9515 • Fax (210) 561-9544  
Toll Free (800) 786-5777  
[www.4adi.com](http://www.4adi.com); [service@4adi.com](mailto:service@4adi.com)

ELISA Kit Components	Amount	Part #
Pneumococcal 23 Type CPS Coated Strip Plate	8-well strips (12)	560-23
Rabbit Anti-Pneumococcal 23 IgG Positive Control	0.65 ml	560-310PC
Anti-Pneumococcal Calibrator 1 U/ml	0.65 ml	560-07-rSB
Anti-Pneumococcal Calibrator 2.5 U/ml	0.65 ml	560-07-rSC
Anti-Pneumococcal Calibrator 5 U/ml	0.65 ml	560-07-rSD
Anti-Pneumococcal Calibrator 10 U/ml	0.65 ml	560-07-rSE
Anti-Human IgG HRP Conjugate (100X)	0.15 ml	H-HuG.211
Sample Diluent (20x)	10 ml	SD20T
Low NSB Sample Diluent	30 ml	TBTm
Wash Solution Concentrate (100X)	10 ml	WB-100
TMB Substrate	12 ml	80091
Stop Solution	12 ml	80101
Product Manual	1 ea	M-560-310-23G


Note: Most non-vaccinated rabbit samples do not contain appreciable non-specific CWPS antibodies and may not have to adsorbed for testing specific CPS antibodies. Please consult: [ADI\\_Res\\_Bull\\_2013\\_Pneumococcal\\_Vaccine\\_tests.pdf](#)

## INTERPRETATION OF RESULTS

### A. Antibody Activity Threshold Index

Compare Samples to 1 U/ml Calibrator or Internal Control  
= Positive/Negative Cut-off.

#### Example:

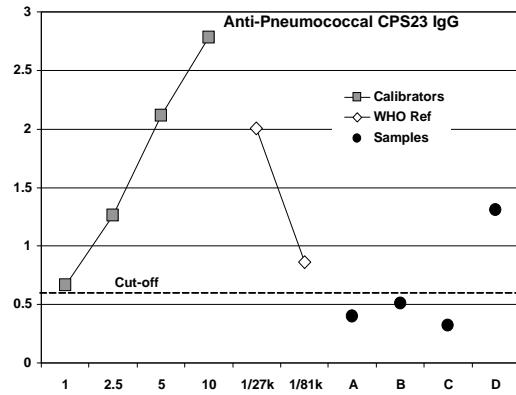

#### Results

The **sensitivity** of the assay to detect anti-Pn 23CPS IgG, from either natural infection or vaccination, is controlled so that the 1 U/ml Calibrator represents a threshold OD for most true positives in human serum diluted to 1:250 or greater. Visual inspection of the data in the above graph shows the following:

**Calibrators** – dilution curve of an anti-Pn 23CPS antiserum, derived from Pn CPS vaccination, shows the OD range of the assay; high value indicates optimal sensitivity of the assay. **1 U/ml:** a 'Cut-off' line has been drawn to indicate a threshold distinguishing between **Positive/Negative**. This is not a clear-cut threshold, rather a low OD area that could represent either low positives or high background negatives.

**WHO Reference Serum** – a pooled serum of individuals vaccinated with Pneumococcal 23CPS (Pneumovax II; Merck; NIBSC code 007sp). **Assay Sensitivity:** the 2.5 U/ml Calibrator = 1/55k dilution of the WHO Reference (CWPS/22F-adsorbed).

**Samples A,B,C,D** – 3 samples (1/250) (A, B, C) are negative: below the threshold; 1 sample (D) is positive: clearly above the threshold.

The 1 U/ml Calibrator can be used to calculate a **Threshold Index** that numerically discriminates Positive/Negative:


- ❖ Divide each Sample net OD by the 1 U/ml Calibrator net OD. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.

## INTERPRETATION OF RESULTS (cont)

### Example (Adsorption of CWPS from samples)

#### Normal Human Serum/Plasma (NHS/P), Adsorbed

A panel of human serum/plasma of unknown history, and the WHO Reference 007sp, were adsorbed with **CWPS/22F** (see page 3) and tested for anti-CPS23 IgG (1/1k dilution) and IgM (1/250 dilution). **Threshold Index** was calculated using the 1 U/ml Cal. Human serum, instead of rabbit serum, is used to show the CWPS testing of adsorbed samples.

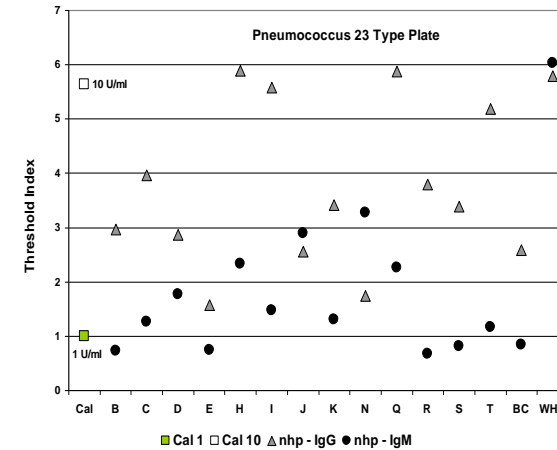

#### Results

**Anti-Pn IgG:** each NHS/P was positive at 1/1k dilution; several NHS/P and the WHO Ref were highly positive.

**Anti-Pn IgM:** many NHS/P were positive at 1/250 dilution; the WHO Ref was highly positive.

**Note:** The CWPS/22F-adsorbed sera can be assayed on plates coated with individual Pn CPS to serotype the positives.

#### B. Positive Index

Experimental sample values may be expressed relative to the values of Control or Non-immune samples, by calculation of a **Positive Index**. One typical method is as follows:

- Calculate the net OD mean + 2 SD of the Control/Non-immune samples = **Positive Index**.
- Divide each sample net OD by the Positive Index. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.


A sample value would be **Positive** if significantly above the value of the pre-immune serum sample or a suitably determined non-immune panel or pool of samples, tested at the same sample dilution.

This calculation also **quantifies** the positive Antibody Activity level, assigning a higher value to samples with higher Antibody Activity, and vice versa.

## INTERPRETATION OF RESULTS (cont)

### C. Antibody Titer

The most accurate method for comparing antibody potencies is by calculation of a titer, using an OD reading midrange in the dilution curves of each antibody as **Index**. In the example below, **IgG** titers were calculated as inverse of the dilution that produced a 1.0 OD in the assay.

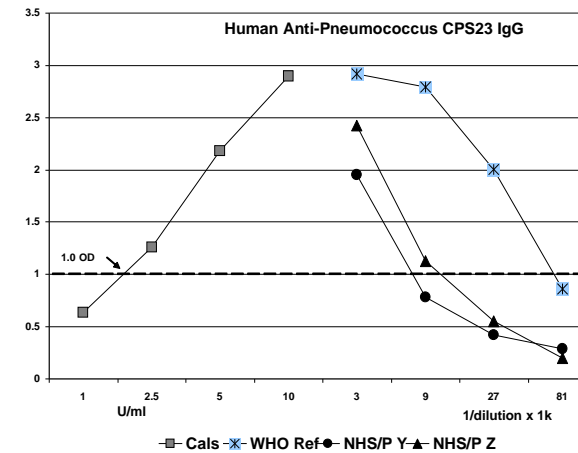

#### Results

**Calibrators:** Titer: 1.7 U/ml. The Calibrator titer value can be used to normalize between-assay sample titer values.

**WHO Reference 007Sp:** a high titer serum pool of individual humans immunized with Pneumococcal 23 CPS-valent vaccine (Pneumovax; Merck). Titer: 80 k

**NHS/P Y:** a normal human plasma of unknown history. Titer: 12 k

**NHS/P Z:** a normal human plasma of unknown history. Titer: 7 k

## PRECAUTIONS AND SAFETY INSTRUCTIONS

Calibrators, Sample Diluent, and Antibody HRP contain bromonitrodioxane (BND: 0.05%, w/v). Stop Solution contains dilute sulfuric acid. Follow good laboratory practices, and avoid ingestion or contact of any reagent with skin, eyes or mucous membranes. All reagents may be disposed of down a drain with copious amounts of water. MSDS for TMB, sulfuric acid and BND can be requested or obtained from the ADI website: [http://4adi.com/commerce/info/showpage.jsp?page\\_id=1060&category\\_id=2430&visit=10](http://4adi.com/commerce/info/showpage.jsp?page_id=1060&category_id=2430&visit=10)