

<b>ELISA Kit Components</b>	<b>Amount</b>	<b>Cat/Part No.</b>
Anti-Rabbit IgM Microwell Strip Plate	8-well strips (12)	6581
Rabbit IgM Control	0.65 ml	6582
Rabbit IgM Standard 10 ng/ml	0.65 ml	6583B
Rabbit IgM Standard 25 ng/ml	0.65 ml	6583C
Rabbit IgM Standard 50 ng/ml	0.65 ml	6583D
Rabbit IgM Standard 100 ng/ml	0.65 ml	6583E
Rabbit IgM Standard 200 ng/ml	0.65 ml	6583F
Anti-Rabbit IgM HRP Conjugate (100X)	0.15 ml	6584
Sample Diluent Concentrate (20X)	10 ml	SD-20T
Wash Solution Concentrate (100X)	10 ml	WB-100
TMB Substrate	12 ml	80091
Stop Solution	12 ml	80101
Product Manual	1 ea	M-6580

## Rabbit IgM ELISA Kit

Cat. No. 6580, 96 Tests

### For Quantitation of Rabbit Immunoglobulin M in Serum, Plasma or Biological Fluids

For research use only (RUO), not for diagnosis, cure or prevention of disease.

#### Related Items

##### Catalog# ProdDescription

1030 Rabbit C-Reactive Protein (CRP) ELISA Kit, 96 tests, Quantitative  
 6390-30 Rabbit Transferrin (Tf) ELISA Kit, 96 tests, Quantitative  
 6510 Rabbit IgA ELISA Kit, 96 tests, Quantitative  
 6580 Rabbit IgG ELISA Kit, 96 tests, Quantitative  
 6580 Rabbit IgM ELISA Kit, 96 tests, Quantitative  
 RDT-3060Rb-10 TruStrip RDT 5-minute Rabbit meat detection/adulteration rapid test cards,  
 6580-RDT-25 TruStrip RDT Rabbit IgG Rapid Test cards  
 7000-30-RDT TruStrip RDT Rabbit Albumin Rapid test cards

For more details please consult our web site ([www.4adi.com](http://www.4adi.com)) or contact us by email ([service@4adi.com](mailto:service@4adi.com)).



**ALPHA DIAGNOSTIC  
INTERNATIONAL**

4638 N Loop 1604 W • San Antonio • Texas 78249 • USA.

Phone (210) 561-9515 • Fax (210) 561-9544

Toll Free (800) 786-5777


Email: [service@4adi.com](mailto:service@4adi.com)

Web Site: [www.4adi.com](http://www.4adi.com)

## INTENDED USE

The Rabbit IgM ELISA Kit is an in vitro immunoassay for the quantification of IgM circulating in serum or in other appropriately qualified samples from tissue fluids (e.g., saliva, mucosa), or in cultures of rabbit cells. For research use only (RUO), not for diagnosis, cure or prevention of the disease.

## RESEARCH USE OF THE TEST



Immunoglobulin G (IgG)


and IgM in the sample and/or individual.

Immunoassays using heavy-chain specific antibodies provide for selective, sensitive quantification of rabbit immunoglobulins IgG, IgA and IgM, as found circulating in blood or as present in other body fluids, including saliva, milk/colostrum, ascites, tears and mucosa of linings of the gut, respiratory or urogenital tracts.

Levels of total IgG, IgA and/or IgM can reveal health status or results of experimental or pathological conditions (e.g., hypo- or hypergammaglobulinemia or acute or chronic infection). Also, measurements of specific antibody levels, in antigen-specific assays, are often best interpreted relative to values of total IgG, IgA,

The quantitative immunoassays measure rabbit IgG and IgM with high sensitivity; this allows dilution beyond interference from the sample matrix for samples derived from any of the above specimen types. Expected performance of each kit relative to precision, recovery and linearity of dilution is presented as guidance for use and experimental design.

## PRINCIPLE OF THE TEST

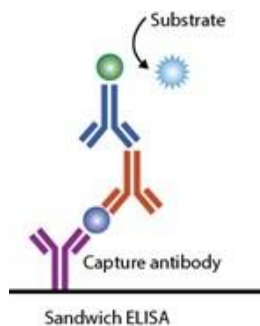

Sandwich ELISA

The Rabbit IgM ELISA kit is based on the binding of Rabbit IgM in samples to two antibodies, one immobilized on the microtiter wells, and the other conjugated to horseradish peroxidase (HRP) enzyme. After a washing step, chromogenic substrate is added and color is developed by the enzymatic reaction of HRP on the TMB substrate, which is directly proportional to the amount of IgM present in the sample. Stopping Solution is added to terminate the reaction, and absorbance at 450nm is then measured using an ELISA microtiter well reader. The concentration of IgM in samples and control is calculated from a curve of standards containing known concentrations of IgM.

## STORAGE AND STABILITY

The microtiter well plate and all other reagents, if unopened, are stable at 2-8°C until the expiration date printed on the box label. Stabilities of the working solutions are indicated under Reagent Preparation.

## PERFORMANCE CHARACTERISTICS

### Specificity

The antibodies used in this kit have been shown by immunoelectrophoresis and ELISA to react specifically with IgM, and have essentially no reactivity with IgG, IgA, IgE or any other rabbit serum proteins.

### Normal Range

Assay of IgM in eighteen (18) sera from individual adult rabbits ranged from **0.32** to **1.50** mg/ml (median = **0.59** mg/ml). Each laboratory should determine expected values of its own testing population.

### Precision

Samples containing low, medium and high concentrations of IgM were assayed as duplicates in multiple assays (n=5) to obtain between-assay reproducibility. Coefficient of variations were calculated for the concentrations using a point-to-point curve-fitting program.

IgM concentrations were measured with good between-assay (**2.1** to **8.9** %CV) reproducibility.

Sample	IgM ng/ml	Inter-assay %CV
Low IgM	35	<b>2.1</b>
Medium IgM	70	<b>3.5</b>
High IgM	128	<b>8.9</b>

### Linearity of Dilution

Six (6) individual stored sera were diluted to 2 levels for testing, and concordance of the assay values were compared. The mean recovery ranged from **91** to **111**%, demonstrating linear dilution and equivalent quantification across the standard range.

Sample	Dilution	Assay Value ng/ml	Serum Value mg/ml	Concordance
Rabbit A	1:8k	69.3	0.55	<b>91 %</b>
	1:24k	19.3	0.46	
Rabbit B	1:8k	74.8	0.60	<b>102 %</b>
	1:24k	23.8	0.57	
Rabbit C	1:8k	99.7	0.80	<b>98 %</b>
	1:24k	32.1	0.77	
Rabbit D	1:8k	70.2	0.56	<b>102 %</b>
	1:24k	24.2	0.58	
Rabbit E	1:8k	166.3	1.33	<b>111 %</b>
	1:24k	68.9	1.65	
Rabbit F	1:8k	188.4	1.51	<b>101 %</b>
	1:24k	63.6	1.53	

## CALCULATION OF RESULTS


- The results may be calculated using any immunoassay software package. The four-parameter curve-fit is recommended. If software is not available, IgM concentrations may be determined as follows:
- Calculate the mean OD of duplicate samples.
- On graph paper plot the mean OD of the standards (y-axis) against the concentration (ng/ml) of IgM (x-axis). Draw the best fit curve through these points to construct the standard curve. A point-to-point construction is most common and reliable.
- The IgM concentrations in unknown samples and controls can be determined by interpolation from the standard curve.
- Multiply the values obtained for the samples by the dilution factor of each sample.
- Samples producing signals higher than the 160 ng/ml standard should be further diluted and re-assayed.

## TYPICAL RESULTS

The following data are for illustration purposes only. A complete standard curve should be run in every assay to determine sample values.

Wells	Standards, Control & Samples	A450 nm	IgM ng/ml
A1, A2	<b>Negative Diluent Control</b>	0.05	0
B1, B2	10 ng/ml <b>Standard</b>	0.28	10
C1, C2	25 ng/ml <b>Standard</b>	0.62	30
D1, D2	50 ng/ml <b>Standard</b>	1.10	60
E1, E2	100 ng/ml <b>Standard</b>	1.81	100
F1, F2	200 ng/ml <b>Standard</b>	2.69	160
G1, G2	<b>Positive IgM Control</b> [Value: 67 - 125 ng/ml]	1.47	76
H1, H2	<b>Sample</b> [Diluted 1:25k] Calculated: 25k-fold dilution x 36 ng/ml = <b>0.9 mg/ml</b> in serum	0.84	36

A typical assay Standard Curve (do not use for calculating sample values)

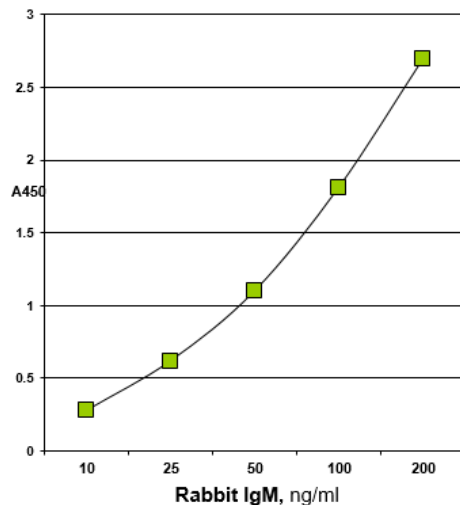

## KIT CONTENTS

**To Be Reconstituted:** Store as indicated.

Component	Instructions for Use
<b>Sample Diluent Concentrate (20x)</b> Cat. No. SD-20T, 10ml	Dilute the entire volume, 10ml + 190ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Sample Diluent</b> and store at 2-8°C until the kit lot expires or is used up.
<b>Wash Solution Concentrate (100x)</b> Cat. No. WB-100, 10ml	Dilute the entire volume 10ml + 990ml with distilled or deionized water into a clean stock bottle. Label as <b>Working Wash Solution</b> and store at RT until kit is used entirely.
<b>Anti-Rabbit IgM - HRP Conjugate Concentrate (100x)</b> Part No. 6584, 0.15ml	Peroxidase conjugated anti-Rabbit IgM in buffer with protein, detergents and antimicrobial as stabilizers. Dilute fresh as needed; 10ul of concentrate to 1ml of <b>Working Sample Diluent</b> is sufficient for 1 8-well strip. Use within the working day and discard. Return concentrate to 2-8°C storage.

**Ready For Use:** Store as indicated on labels.

Component	Part No.	Amt	Contents
<b>Anti-Rabbit IgM Microwell Strip Plate</b>	6581	8-well strips (12)	Coated with purified anti-rabbit IgM antibodies.
<b>Rabbit IgM Standards</b>			
10 ng/ml	6583B	0.65 ml	Five (5) vials, each containing calibrated rabbit IgM in buffer with protein, detergents and antimicrobial as stabilizers.
25 ng/ml	6583C	0.65 ml	
50 ng/ml	6583D	0.65 ml	
100 ng/ml	6583E	0.65 ml	
200 ng/ml	6583F	0.65 ml	
<b>Positive Control [IgM]</b> range on label	6582	0.65 ml	Rabbit IgM diluted in buffer with protein, detergents and antimicrobial as stabilizers.
<b>TMB Substrate</b>	80091	12 ml	Chromogenic substrate for HRP containing TMB and peroxide.
<b>Stop Solution</b>	80101	12 ml	1% sulfuric acid.

#### Materials Required But Not Provided:

- Pipettors and pipettes that deliver 100ul and 1-10ml. A multi-channel pipettor is recommended.
- Disposable glass or plastic 5-15ml tubes for diluting samples and Anti-Rabbit IgM-HRP Concentrate.
- Graduated cylinder to dilute Wash Concentrate and Sample Diluent concentrate; 200ml to 1L.
- Stock bottle to store diluted Wash Solution; 200ml to 1L.
- Distilled or deionized water to dilute reagent concentrates.
- Microwell plate reader at 450 nm wavelength.

#### SPECIMEN COLLECTION AND HANDLING

Collect blood by venipuncture, allow clotting, and separate the serum by centrifugation at room temperature. Do not heat inactivate the serum. If sera are not assayed immediately, store refrigerated for up to 2 weeks, or frozen for long-term storage. The use of plasma has not been investigated, but should be a suitable specimen for assay.

#### PRECAUTIONS AND SAFETY INSTRUCTIONS

Standards, Controls, Sample Diluent, and Anti-Rabbit IgM-HRP contain Bromo-nitro-dioxane (BND: 0.05%, w/v). Stop Solution contains 1% sulfuric acid. Follow good laboratory practices, and avoid ingestion or contact of any reagent with skin, eyes or mucous membranes. All reagents may be disposed of down a drain with copious amounts of water. Applicable **MSDS**, if not already on file, for the following reagents can be obtained from ADI or the web site.

[http://4adi.com/commerce/info/showpage.jsp?page\\_id=1060&category\\_id=2430&visit=10](http://4adi.com/commerce/info/showpage.jsp?page_id=1060&category_id=2430&visit=10)

#### QUALITY CONTROL

**Reagents** Accurate and reproducible assay results rely on proper storage, handling and control of reagent and sample temperature. Store all reagents as indicated, and warm to room temperature only those to be used in the assay. Shelf-life of the critical reagents and samples will diminish with extended exposure to non-refrigeration, resulting in inaccurate assay results. All solutions should be clear. Cloudiness or particulates are indications of reagent contamination or instability and may interfere with proper performance of the assay. Do not use.

**Sample Controls** A Positive Serum Control is provided with the kit, assigned with an IgM concentration value range. Recovery in this range is an indicator of proper assay performance. Each lab should also assay internal control samples, which represent the lab's expected sample population and that are maintained stabilized. A Negative Diluent Control should also be run; OD < 0.3.

**Standard Curve** The signal generated by the standards should be continuously increasing in OD from the lowest Standard to the highest Standard, with a difference greater than 1.2 OD. Non-continuously increasing or low signals may indicate problems with technique, protocol directions and/or reagent preparation, use or stability. A Negative Diluent Control should be of lower signal than the lowest standard. Do not rely on results generated from an assay with these issues.

**Technique** Accurate and reproducible assay results rely on good lab technique regarding pipetting, plate washing and handling of samples and reagents.

**Equipment** Precision of results relies on uniform and effective washing techniques; an automatic washer is recommended. ELISA reader and pipettes should be properly calibrated.

#### ASSAY PROCEDURE

Bring all reagents to room temperature (18-30° C) equilibration (at least 30 minutes).

DILUTE Serum Samples in Working Sample Diluent. Dilutions of about 1:10,000 are appropriate for most normal rabbit sera. For accuracy, three dilution steps are recommended, as follows:

- 1) 10ul serum + 990ul diluent = [1:100],
- 2) 10ul [1:100] + 990ul diluent = **1:10,000**

DO NOT dilute the Standards or Control.

ALL STEPS ARE PERFORMED AT ROOM TEMPERATURE. After each reagent addition, gently tap the plate to mix the well contents prior to beginning incubation.

##### 1. **Set-up**

Determine the number of wells for the assay run. Duplicates are recommended, including 10 Standard wells and 2 wells for each sample and control to be assayed.

- Remove the appropriate number of microwell strips from the pouch and return unused strips to the pouch. Reseal the pouch and store refrigerated.
- Add 200-300ul Working Wash Solution to each well and let stand for 5 to 30 minutes before sample addition.
- Aspirate the liquid and pat dry on a paper towel.

##### 2. **1<sup>st</sup> Incubation** [100ul – 60 min; 4 washes]

- Add 100ul of standards, samples and controls each to pre-determined wells.
- Tap the plate gently to mix reagents and incubate for 60 minutes.
- Wash wells 4 times and pat dry on fresh paper towels. As an alternative, an automatic plate washer is recommended. Improper washes may lead to falsely elevated signals and poor reproducibility.

##### 3. **2<sup>nd</sup> Incubation** [100ul – 30 min; 5 washes]

- Add 100ul of diluted Anti-Rabbit IgM-HRP Conjugate to each well.
- Incubate for 30 minutes.
- Wash wells 5 times as in step 2.

##### 4. **Substrate Incubation** [100ul – 15 min]

- Add 100ul TMB Substrate to each well. The liquid in the wells will begin to turn blue.
- Incubate for 15 minutes in the dark, e.g., place in a drawer or closet.  
Note: If your microplate reader does not register optical density (OD) above 2.0, incubate for less time, assuring the top standard does not surpass 2 OD.

##### 5. **Stop Step** [Stop: 100ul]

- Add 100ul of Stop Solution to each well.
- Tap gently to mix. The enzyme reaction will stop; liquid in the wells will turn yellow.

##### 6. **Absorbance Reading**

- Use any commercially available microplate reader capable of reading at 450nm wavelength. Use a program suitable for obtaining OD readings, and data calculations if available.
- Read absorbance of the entire plate at 450nm using a single wavelength within 30 minutes after Stop Solution addition. If available, program to subtract OD at 630nm to normalize well background.